

RESEARCH OUTPUTS / RÉSULTATS DE RECHERCHE

Poly(ether ether ketone) (PEEK) XPS reference core level and energy loss spectra

Louette, Pierre; Bodino, Frédéric; Pireaux, Jean-Jacques

Published in:
Surface science spectra

Publication date:
2005

Document Version
Early version, also known as pre-print

[Link to publication](#)

Citation for published version (HARVARD):

Louette, P, Bodino, F & Pireaux, J-J 2005, 'Poly(ether ether ketone) (PEEK) XPS reference core level and energy loss spectra', *Surface science spectra*, vol. 12, pp. 149-153.

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal ?

Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Poly(ether ether ketone) (PEEK) XPS Reference Core Level and Energy Loss Spectra

Pierre Louette,^{a)} Frederic Bodino, and Jean-Jacques Pireaux
University of Namur - LISE, 61, Rue de Bruxelles, B-5000 Namur, Belgium

(Received 21 October 2005; accepted 6 June 2006; published 16 February 2007)

XPS measurements of poly(ether ether ketone) recorded with a SSX-100 spectrometer in standardized experimental conditions are presented: survey scan, high resolution core level spectra as well as the energy loss regions of carbon and oxygen peaks are analyzed. This is part of a contract work aiming to record spectra in the very same conditions of some 40 different polymers. © 2006 American Vacuum Society. [DOI: 10.1116/11.20051106]

Keywords: *x-ray photoelectron spectroscopy; XPS; surface; polymer; poly(ether ether ketone); PEEK*

PACS: 79.60.Fr, 82.80.Pv, 79.20.Uv, 61.41.+e, 01.30.Kj

SPECIMEN DESCRIPTION

Host Material: poly(ether ether ketone)

CAS Registry #: 31694-16-3

Host Material Characteristics: homogeneous; solid; amorphous; dielectric; polymer


Chemical Name: poly(ether ether ketone)

Source: ICI

Host Composition: not specified

Form: pellet

Structure:



History & Significance: This study is a part of a reference spectra database of polymers, including survey and core level spectra, but also energy loss spectra of the main elements.

As Received Condition: not specified

Analyzed Region: same as host material

Ex Situ Preparation/Mounting: pressed powder

In Situ Preparation: none

Pre-Analysis Beam Exposure: The analyzed region was exposed to x-rays for a very short time, around 2 min for sample position adjustment prior to measurements.

Charge Control: use of a metal screen and a flood gun (2 eV)

Temp. During Analysis: 300 K

Pressure During Analysis: $<6.6 \times 10^{-8}$ Pa

INSTRUMENT DESCRIPTION

Manufacturer and Model: Surface Science Instruments SSX-100

Analyzer Type: spherical sector

Detector: position sensitive detector with microchannel plate

^{a)} Author to whom correspondence should be addressed.

Accession # 00891

Technique: XPS

Host Material: poly(ether ether ketone)

Instrument: Surface Science Instruments SSX-100

Major Elements in Spectrum: C, O

Minor Elements in Spectrum: none

Printed Spectra: 5

Spectra in Electronic Record: 5

Spectral Category: comparison

Number of Detector Elements: 128

INSTRUMENT PARAMETERS COMMON TO ALL SPECTRA

■ Spectrometer

Analyzer Mode: constant pass energy

Throughput ($T = E^N$): $N =$ See comment below

Throughput Comment: $T = E^N$, $N = 0.7$

Excitation Source Window: 1.5 μm Al foil

Excitation Source: Al K_{α} monochromatic

Source Energy: 1486.6 eV

Source Strength: 130 W

Source Beam Size: 0.6 mm \times 0.6 mm

Signal Mode: not specified

■ Geometry

Incident Angle: 57.6°

Source to Analyzer Angle: 70.8°

Emission Angle: 14.7°

Specimen Azimuthal Angle: 75.5°

Acceptance Angle from Analyzer Axis: 0°

Analyzer Angular Acceptance Width: 30° \times 30°

DATA ANALYSIS METHOD

Energy Scale Correction: To compensate for charging effects, we adjusted the largest C 1s component to 284.70 eV (Ref. 1).

Recommended Energy-Scale Shift: +6.03 eV

Peak Shape and Background Method: A least square fitting routine with mixed Gaussian/Lorentzian for the components and a linear background was used.

Quantitation Method: Scofield factors corrected for energy dependence were used.

ACKNOWLEDGMENTS

This study is a part of the EU-BCR contract "XPS Spectral Intensity Data Bank." We thank the NPL for authorizing us to publish these spectra.

REFERENCES


1. G. Beamson and D. Briggs, in *The Scienta ESCA 300 Database* (Wiley, Chichester, 1992).

2. C. J. Powell, *J. Electron. Spectrosc. Relat. Phenom.* **47**, 197 (1988).

SPECTRAL FEATURES TABLE

Spectrum ID #	Element/Transition	Peak Energy (eV)	Peak Width FWHM (eV)	Peak Area (eV-cts/s)	Sensitivity Factor	Concentration (at. %)	Peak Assignment
00891-02	C 1s	284.70	1.11	7815	1.00	64.5	1 in Diagram below
00891-02	C 1s	286.31	1.09	1915	1.00	16.0	2 in Diagram below
00891-02	C 1s	287.10	0.94	213	1.00	1.8	3 in Diagram below
00891-02	C 1s	291.59	1.81	405	1.00
00891-03	O 1s	531.31	1.42	1445	2.49	4.9	4 in Diagram below
00891-03	O 1s	533.40	1.30	3542	2.49	11.9	5 in Diagram below
00891-03	O 1s	540.91	3.29	154	2.49

Comment to Spectral Features Table:




ANALYZER CALIBRATION TABLE

Spectrum ID #	Element/Transition	Peak Energy (eV)	Peak Width FWHM (eV)	Peak Area (eV-cts/s)	Sensitivity Factor	Concentration (at. %)	Peak Assignment
...	Cu 2p _{3/2}	932.34	1.19	202906	9.748
...	Cu 3p _{3/2}	74.78	2.36	289045	2.774


GUIDE TO FIGURES

Spectrum (Accession) #	Spectral Region	Voltage Shift*	Multiplier	Baseline	Comment #
891-1	Survey	-6.03	1	0	
891-2	C 1s	-6.03	1	0	
891-3	O 1s	-6.03	1	0	
891-4	C 1s + losses	-6.03	1	0	
891-5	O 1s + losses	-6.03	1	0	

* Voltage shift of the archived (as-measured) spectrum relative to the printed figure. The figure reflects the recommended energy scale correction due to a calibration correction, sample charging, flood gun, or other phenomenon.

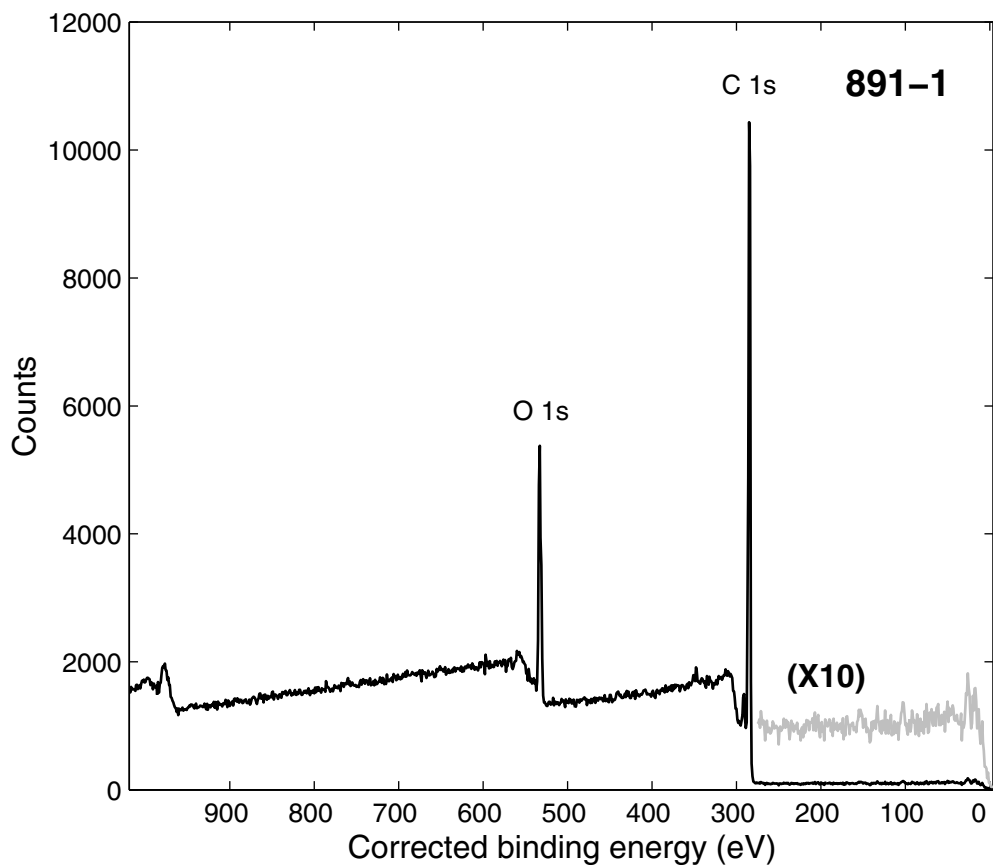


Accession #	00891-01
Host Material	poly(ether ether ketone)
Technique	XPS
Spectral Region	survey
Instrument	Surface Science Instruments SSX-100
Excitation Source	Al K_{α} monochromatic
Source Energy	1486.6 eV
Source Strength	130 W
Source Size	0.6 mm \times 0.6 mm
Analyzer Type	spherical sector
Incident Angle	57.6°
Emission Angle	14.7°
Analyzer Pass Energy	106.8 eV
Analyzer Resolution	1.17 eV
Total Signal Accumulation Time	960 s
Total Elapsed Time	not specified
Number of Scans	2
Effective Detector Width	12.96 eV

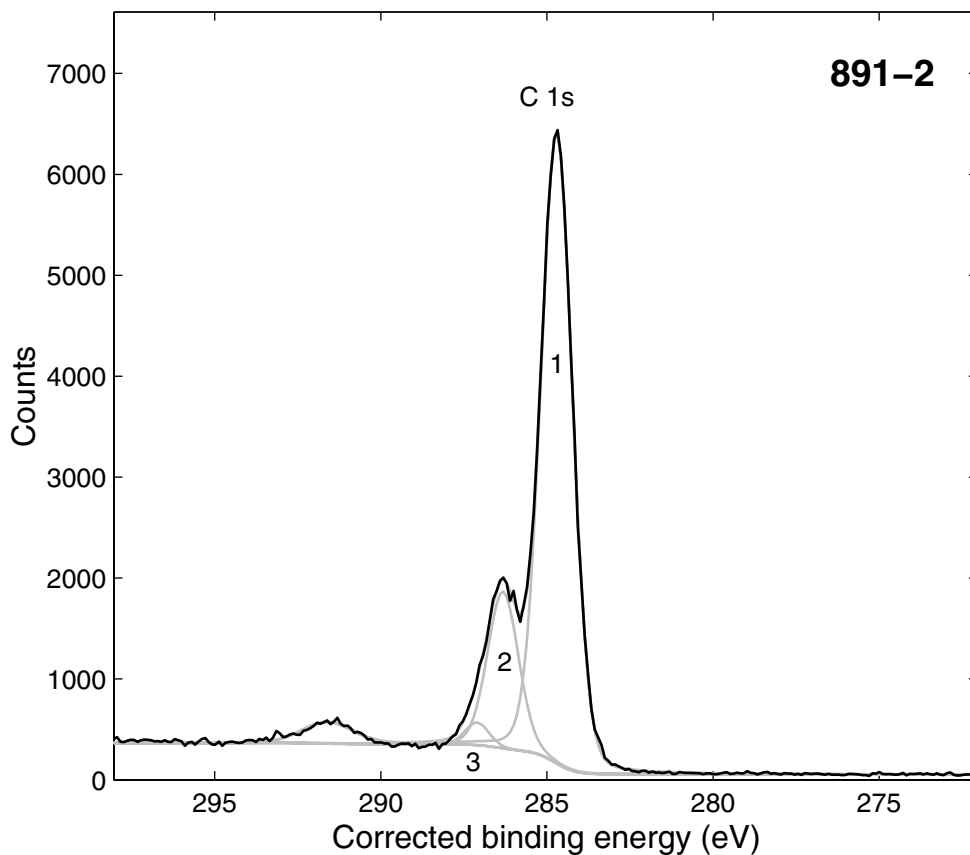


■ **Accession #:** 00891-02
 ■ **Host Material:** poly(ether ether ketone)
 ■ **Technique:** XPS
 ■ **Spectral Region:** C 1s

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 130 W
 Source Size: 0.6 mm \times 0.6 mm
 Incident Angle: 57.6°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 29.97 eV
 Analyzer Resolution: 0.76 eV
 Emission Angle: 14.7°
 Total Signal Accumulation Time: 1200 s
 Total Elapsed Time: not specified
 Number of Scans: 10
 Effective Detector Width: 3.341 eV

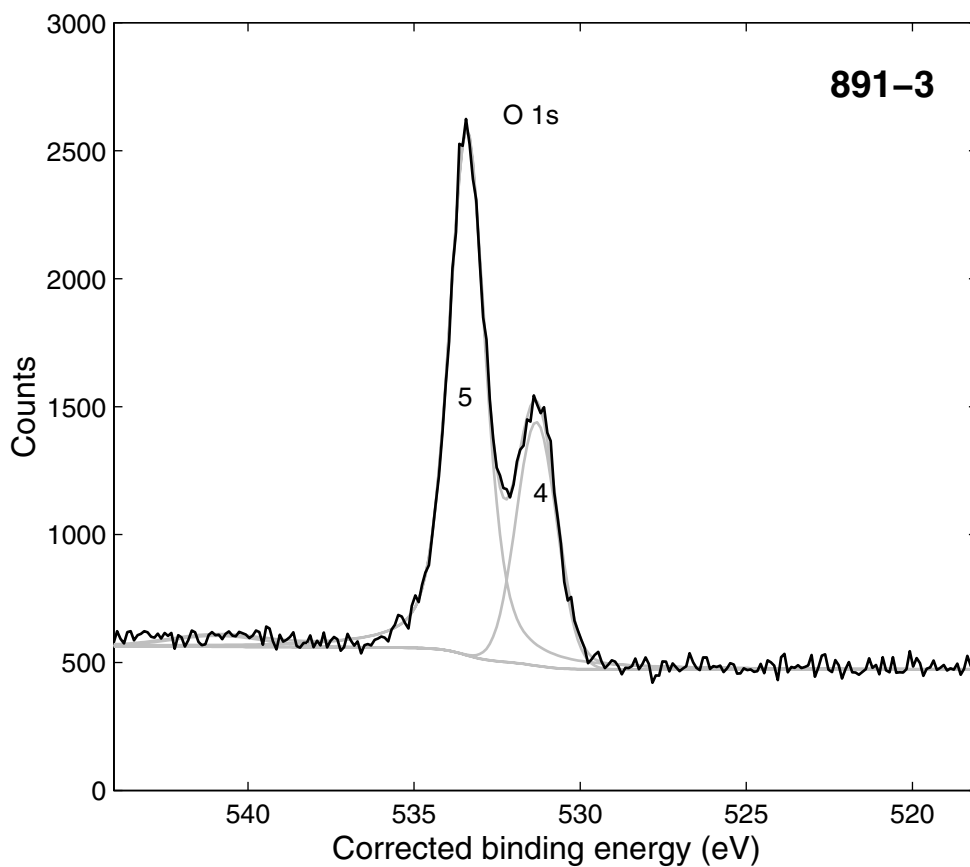


■ **Accession #:** 00891-03
 ■ **Host Material:** poly(ether ether ketone)
 ■ **Technique:** XPS
 ■ **Spectral Region:** O 1s

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 130 W
 Source Size: 0.6 mm \times 0.6 mm
 Incident Angle: 57.6°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 29.97 eV
 Analyzer Resolution: 0.76 eV
 Emission Angle: 14.7°
 Total Signal Accumulation Time: 1200 s
 Total Elapsed Time: not specified
 Number of Scans: 10
 Effective Detector Width: 3.341 eV

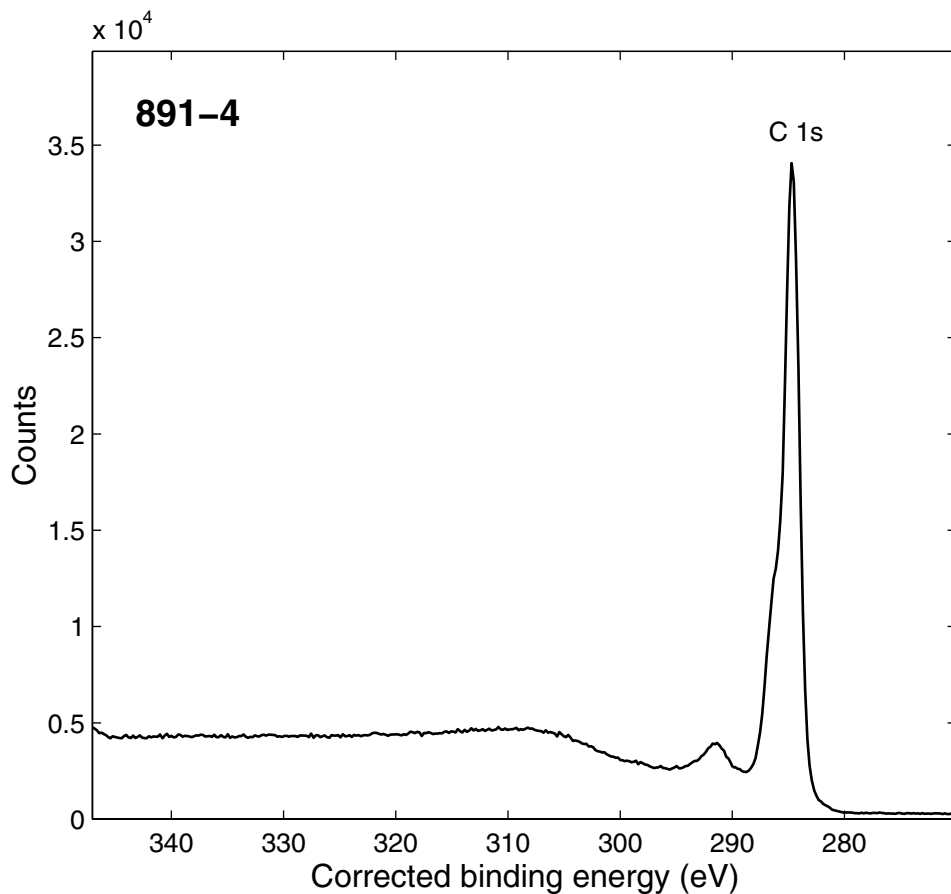

■ **Accession #:** 00891-04
 ■ **Host Material:** poly(ether ether ketone)
 ■ **Technique:** XPS
 ■ **Spectral Region:** C 1s energy losses

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 130 W
 Source Size: 0.6 mm \times 0.6 mm
 Incident Angle: 57.6°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 106.8 eV
 Analyzer Resolution: 1.17 eV
 Emission Angle: 14.7°
 Total Signal Accumulation Time: 900 s
 Total Elapsed Time: not specified
 Number of Scans: 5
 Effective Detector Width: 12.956 eV

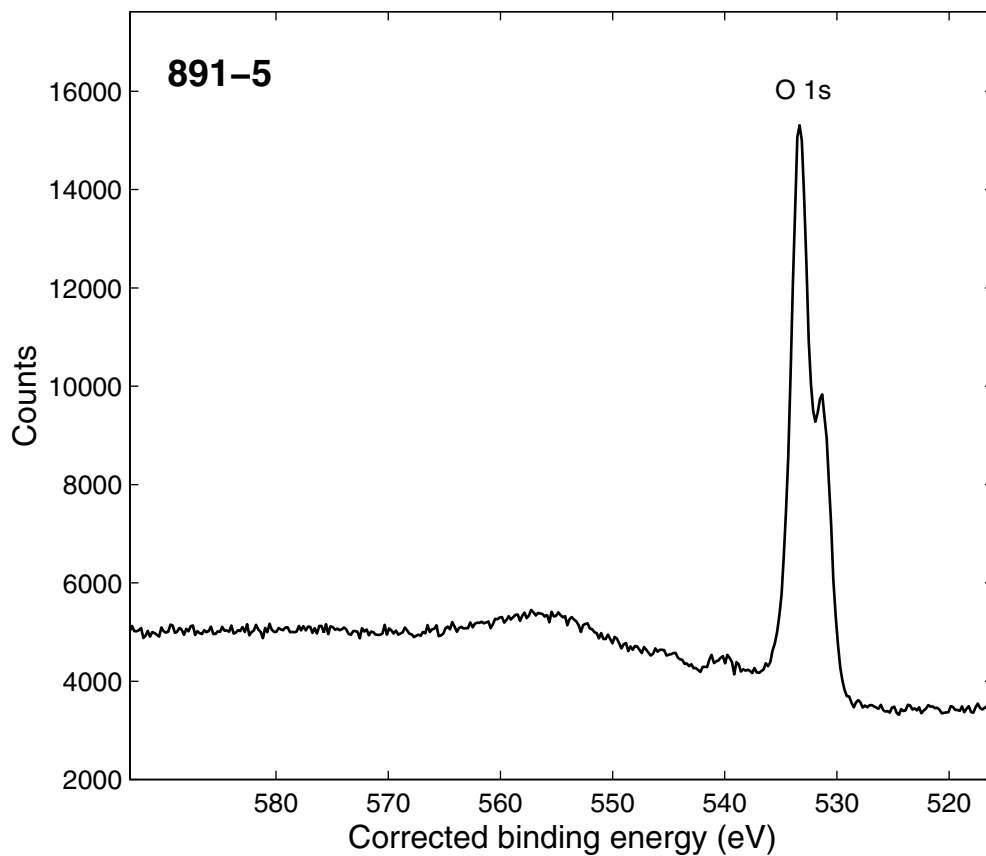

■ **Accession #:** 00891-05
 ■ **Host Material:** poly(ether ether ketone)
 ■ **Technique:** XPS
 ■ **Spectral Region:** O 1s energy losses

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 130 W
 Source Size: 0.6 mm \times 0.6 mm
 Incident Angle: 57.6°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 106.8 eV
 Analyzer Resolution: 1.17 eV
 Emission Angle: 14.7°
 Total Signal Accumulation Time: 900 s
 Total Elapsed Time: not specified
 Number of Scans: 5
 Effective Detector Width: 12.956 eV