

## RESEARCH OUTPUTS / RÉSULTATS DE RECHERCHE

### **Elaboration of tantalum oxide and carbon nanotubes composite coatings on titanium for biomaterial applications**

Maho, Anthony; Linden, Stéphanie; Arnould, Christelle; Detriche, Simon; Delhalle, Joseph; Mekhalif, Zineb

*Publication date:*  
2011

*Document Version*  
Peer reviewed version

[Link to publication](#)

*Citation for published version (HARVARD):*

Maho, A, Linden, S, Arnould, C, Detriche, S, Delhalle, J & Mekhalif, Z 2011, 'Elaboration of tantalum oxide and carbon nanotubes composite coatings on titanium for biomaterial applications', ElecNano4- 7th ECHEMS, Paris, France, 23/05/11 - 26/05/11.

#### **General rights**

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal ?

#### **Take down policy**

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.



# Elaboration of tantalum oxide and carbon nanotubes composite coatings on titanium for biomaterial applications

**Anthony Maho**, Stéphanie Linden, Christelle Arnould, Simon Detriche, Joseph Delhalle, Zineb Mekhalif  
 Laboratory of Chemistry and Electrochemistry of Surfaces (CES)  
 University of Namur (FUNDP), Belgium  
 Contact: zineb.mekhalif@fundp.ac.be

## General context: titanium-based biomaterials

- Titanium and its alloys** constitute very interesting and useful platforms for **dental and osseous biomedical applications** thanks to their low density, high fatigue strength, inertness to human body, corrosion resistance, ... However, toxicity of certain alloying elements (Ni in Nitinol, ...), long-term degradation and weak osseointegration remain problematic features [1].
- One solving approach => formation of a **thin tantalum coating** on Ti surface by **sol-gel** process: Ta, with its very passivating oxide layer, is highly resistant to corrosion, biocompatible and bioactive, has good radio-opacity, ... Nevertheless, high price and important density restrict its use as a bulk material [2].
- Multiwalled **carbon nanotubes (MWCNTs)** can be incorporated to form a **composite Ta-based coating** on Ti owing to their ability to improve the mechanical properties of the implant. They can also **specifically interact with osteoblasts and osteoclasts** and promote the bone regeneration process by **mimicking the structure of collagen fibers** and **favor the formation of an hydroxyapatite layer** [3].
- Hydroxyapatite formation can also be favored by the presence of **molecular films of amino-tris-methylene phosphonic acid** on the  $Ta_2O_5$ -based surface. The utilization of such **multifunctional phosphonic acid molecules** is of particular interest, as some  $-PO_3H_2$  functions can be used as strong anchoring feet with the metallic oxide surface while others, acting as terminal groups, directly favor the hydroxyapatite growth at the interface with body environment [4].


## Global strategy

(A) **Sol-gel co-deposition of  $Ta_2O_5$ /MWCNTs composite coatings on Ti substrates: optimized treatment**

- => **10 min immersion in a sol-gel solution** made of 4.0 mL abs. EtOH, 0.2 mL of HCl (acid catalyst), and 8.0 mg of oxidized MWCNTs
- => **10 min gradual hydrolysis** in distilled water
- => **3 min drying at 300°C**

(B) **Grafting of an amino-tris-methylene phosphonic acid layer: 1 h immersion** in a  $10^{-3}$  M  $N(CH_2PO_3H_2)_3$  aqueous solution at 25°C and pH~1



(C) ***In vitro* hydroxyapatite surfacial growth: 7 days immersion** in 30 mL of a **Simulated Body Fluid** at 37°C and pH 7.25

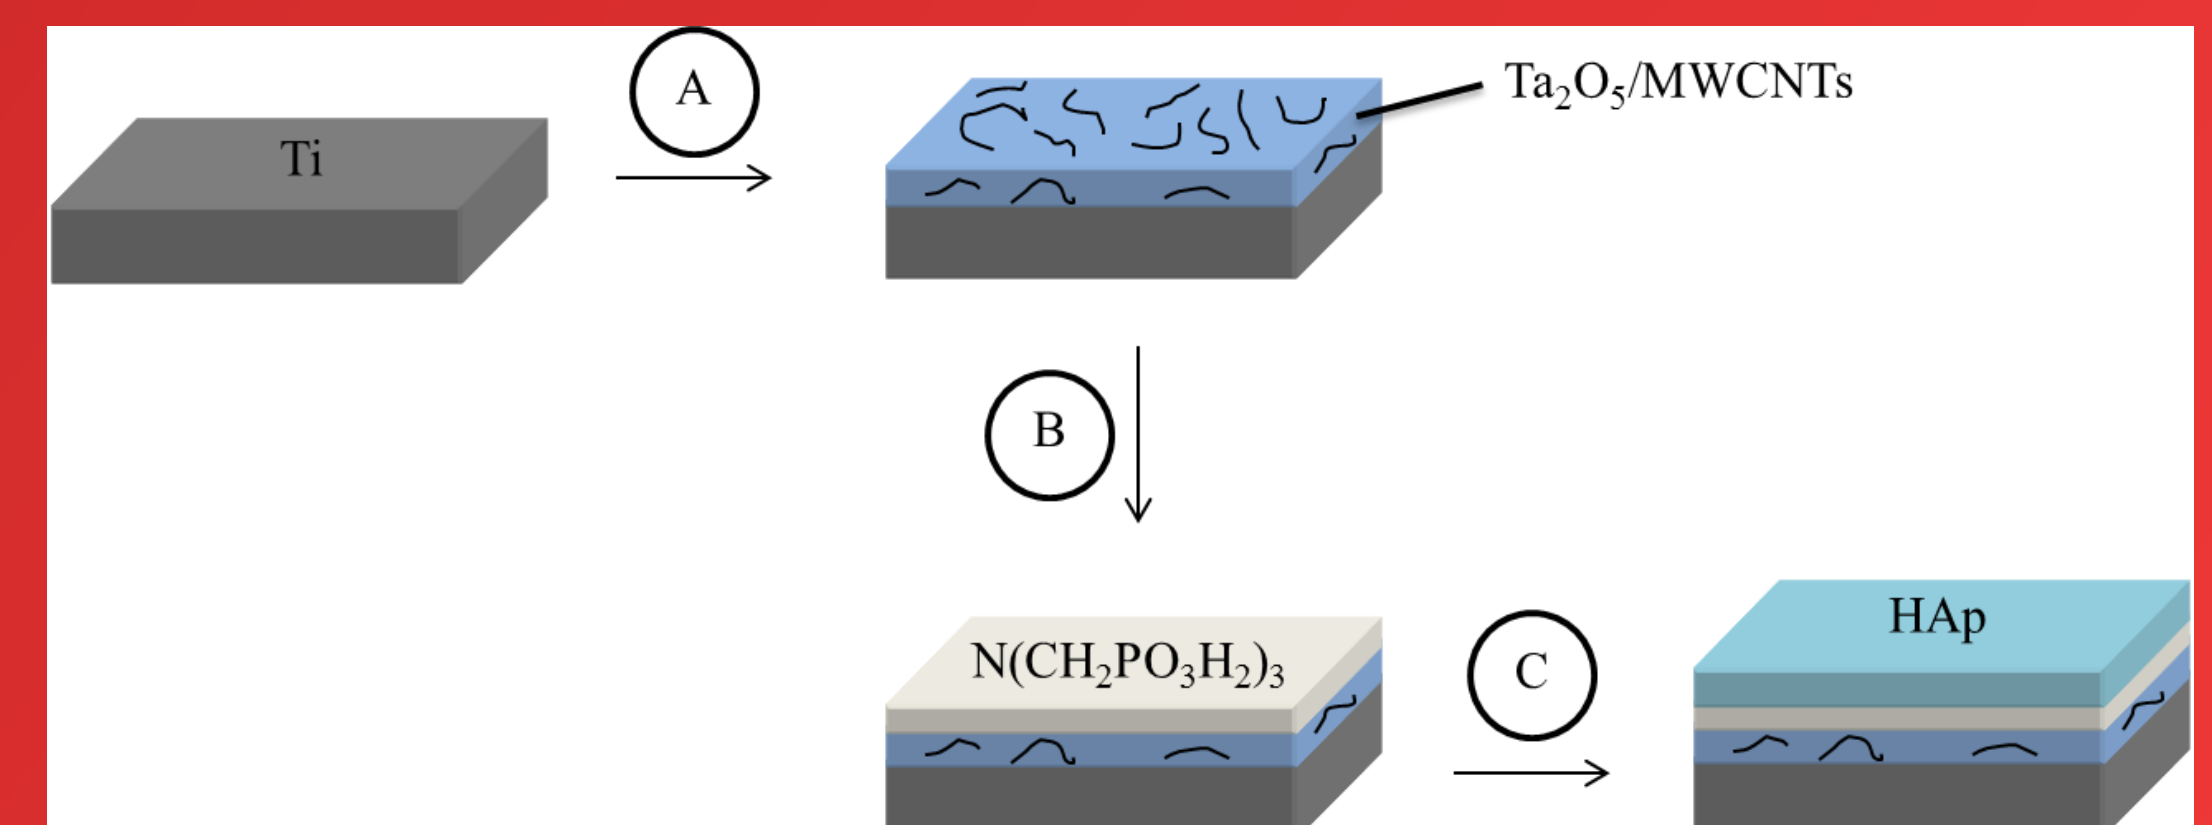

## Results and discussion





### MWCNTs oxidative treatment

- Optimized procedure:** oxidation in a **0.1 M  $KMnO_4/H_2SO_4$  mixture at 60°C during 2 h**
  - => MWCNTs are soluble in abs. EtOH
  - => Oxidation of MWCNTs is confirmed by XPS (C1s signal)
  - => A global moderate shortening of the tubes is observed (length distributions out of TEM characterizations)

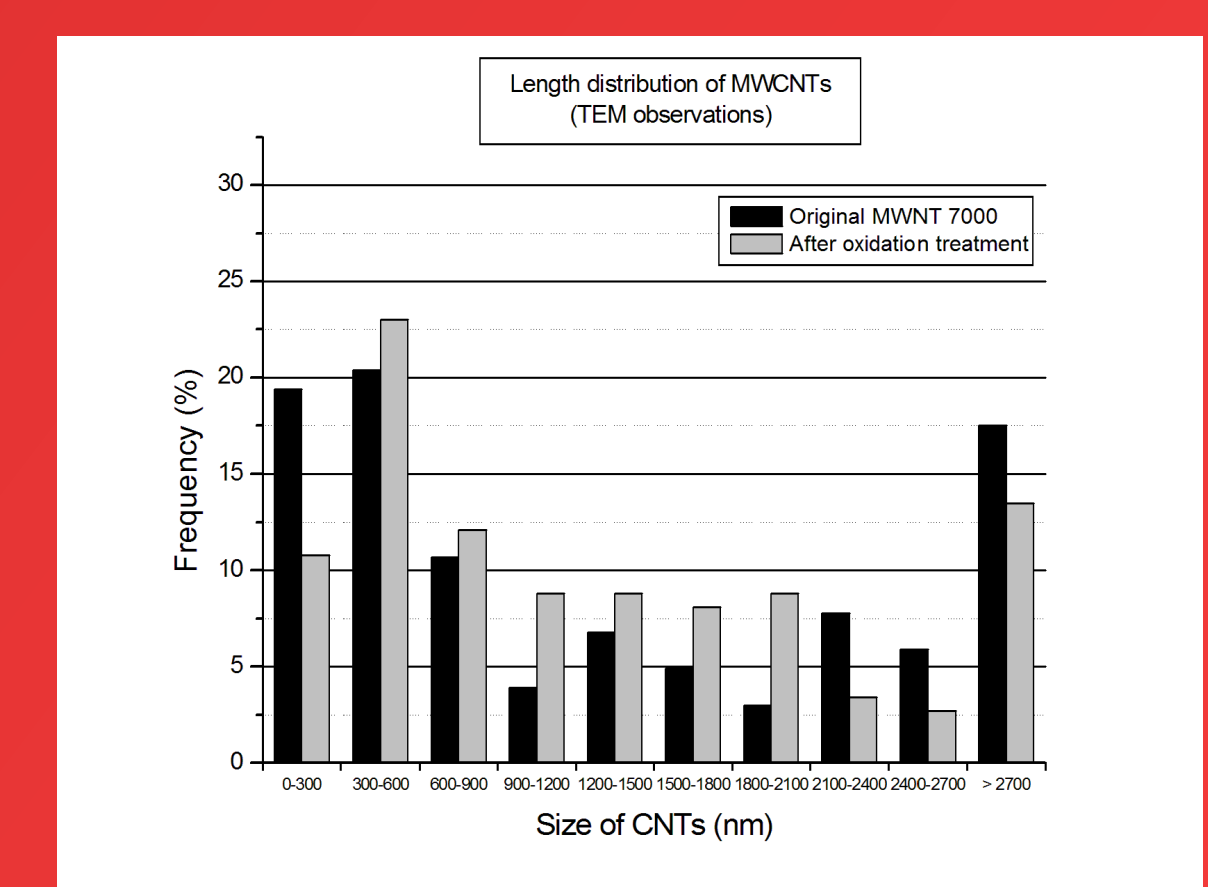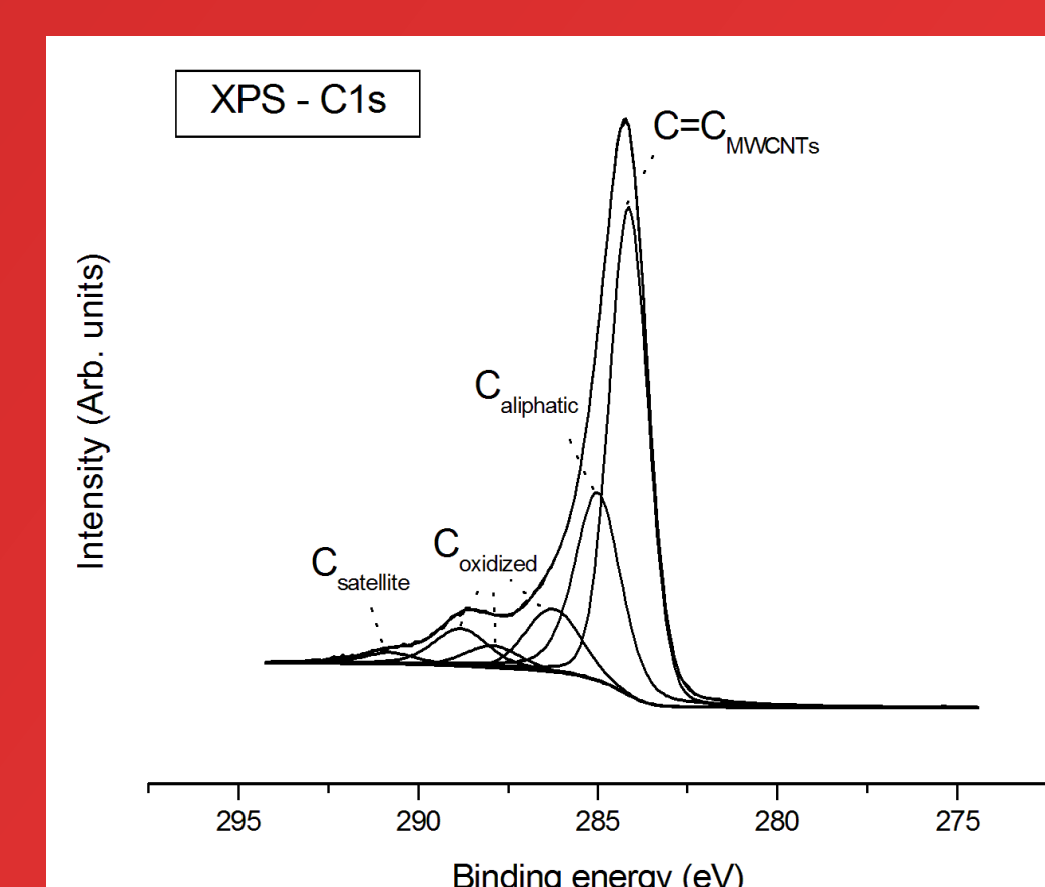




### Sol-gel co-deposition of $Ta_2O_5$ /MWCNTs composite coatings on Ti (A)

- Formation of **uncracked, adherent and homogeneous deposits** (XPS, SEM)
- Passivation and high corrosion resistance** are observed with composite coatings (free potential, polarization curves)

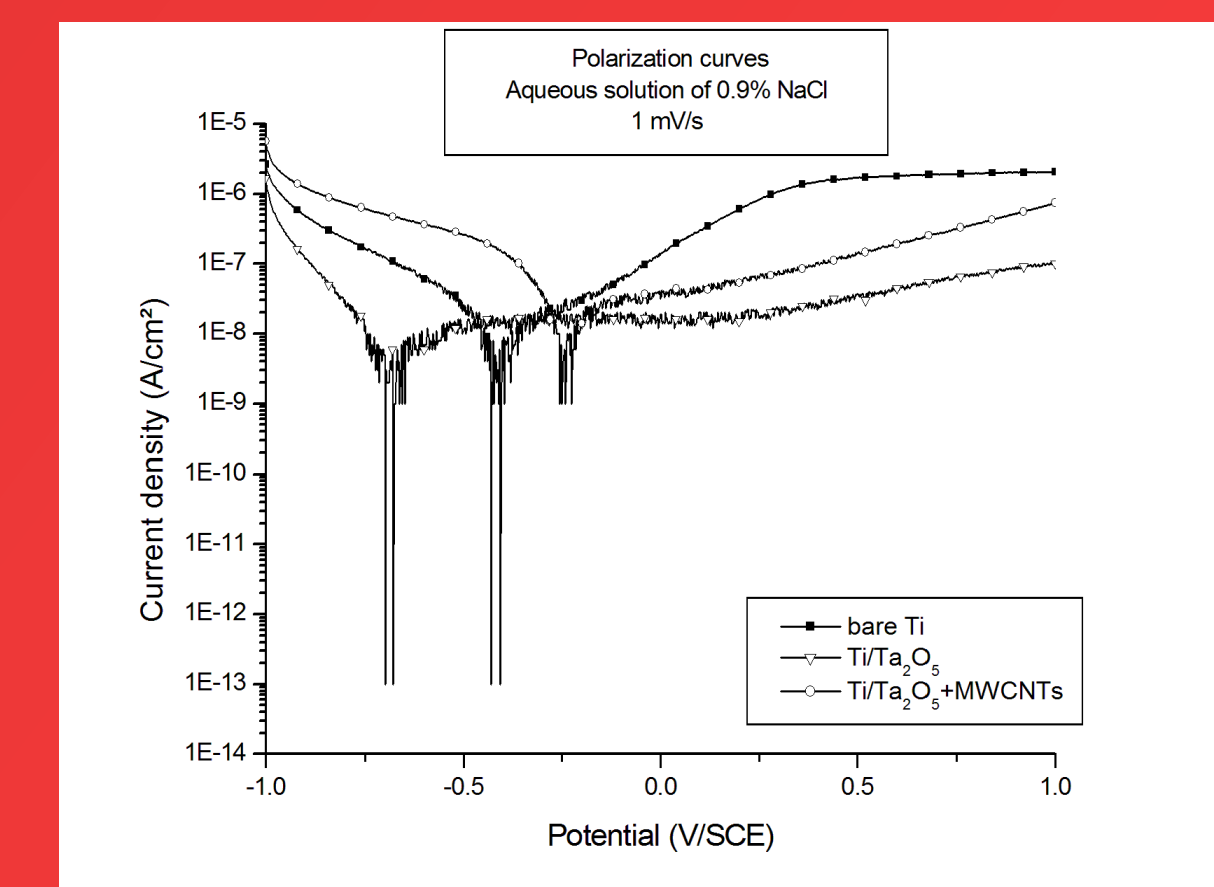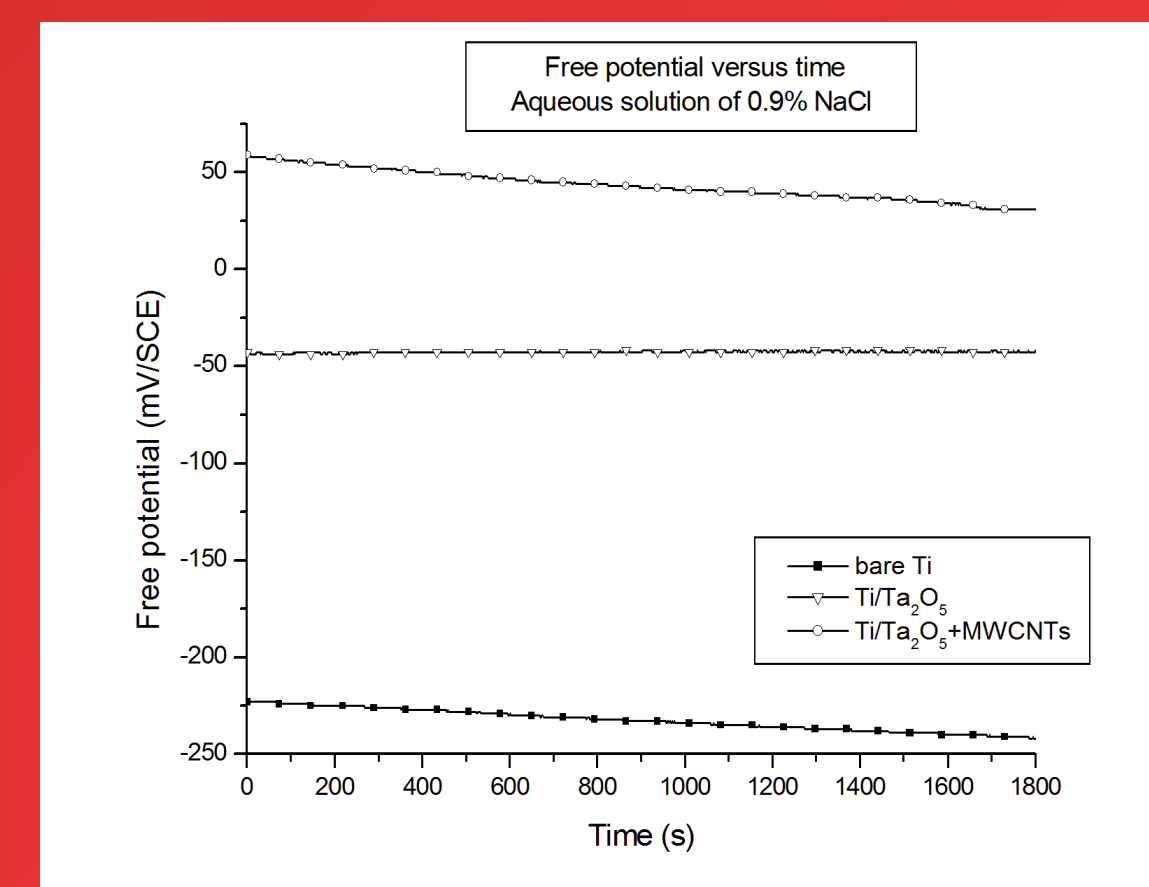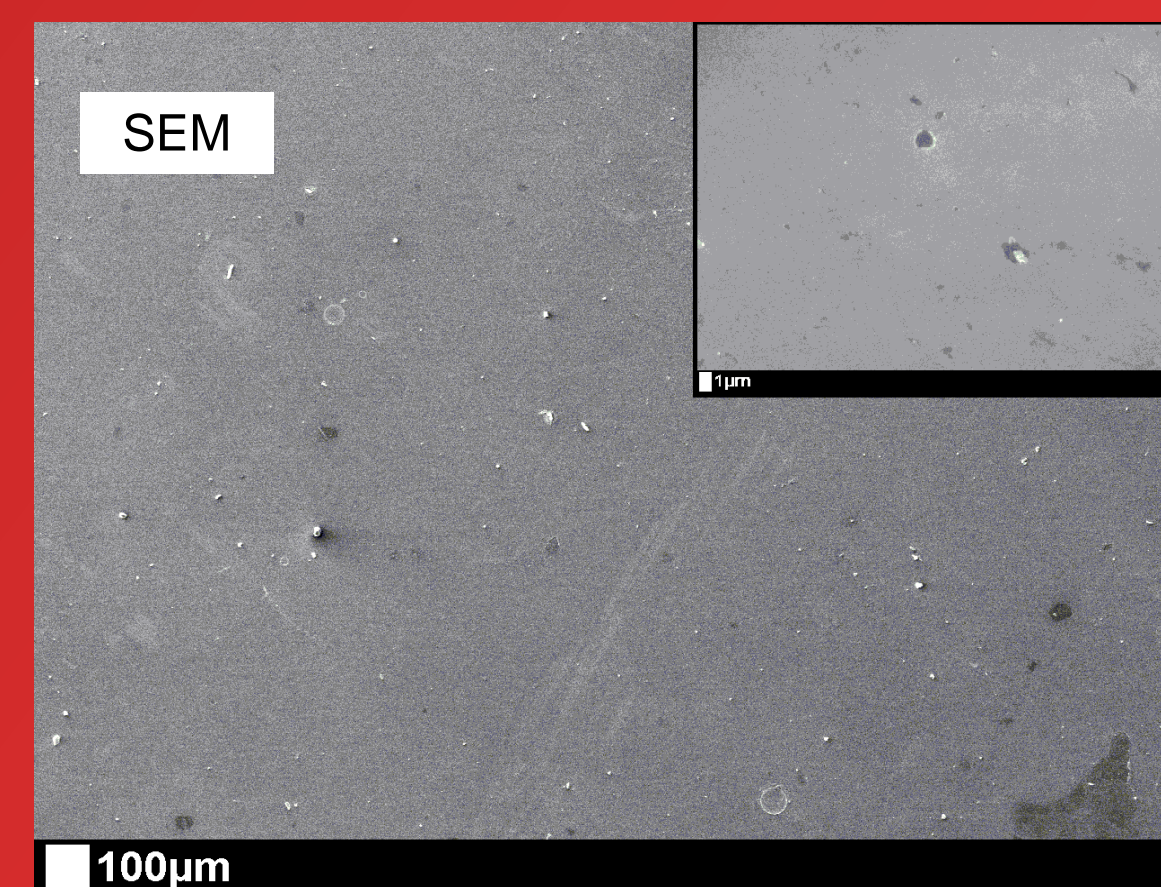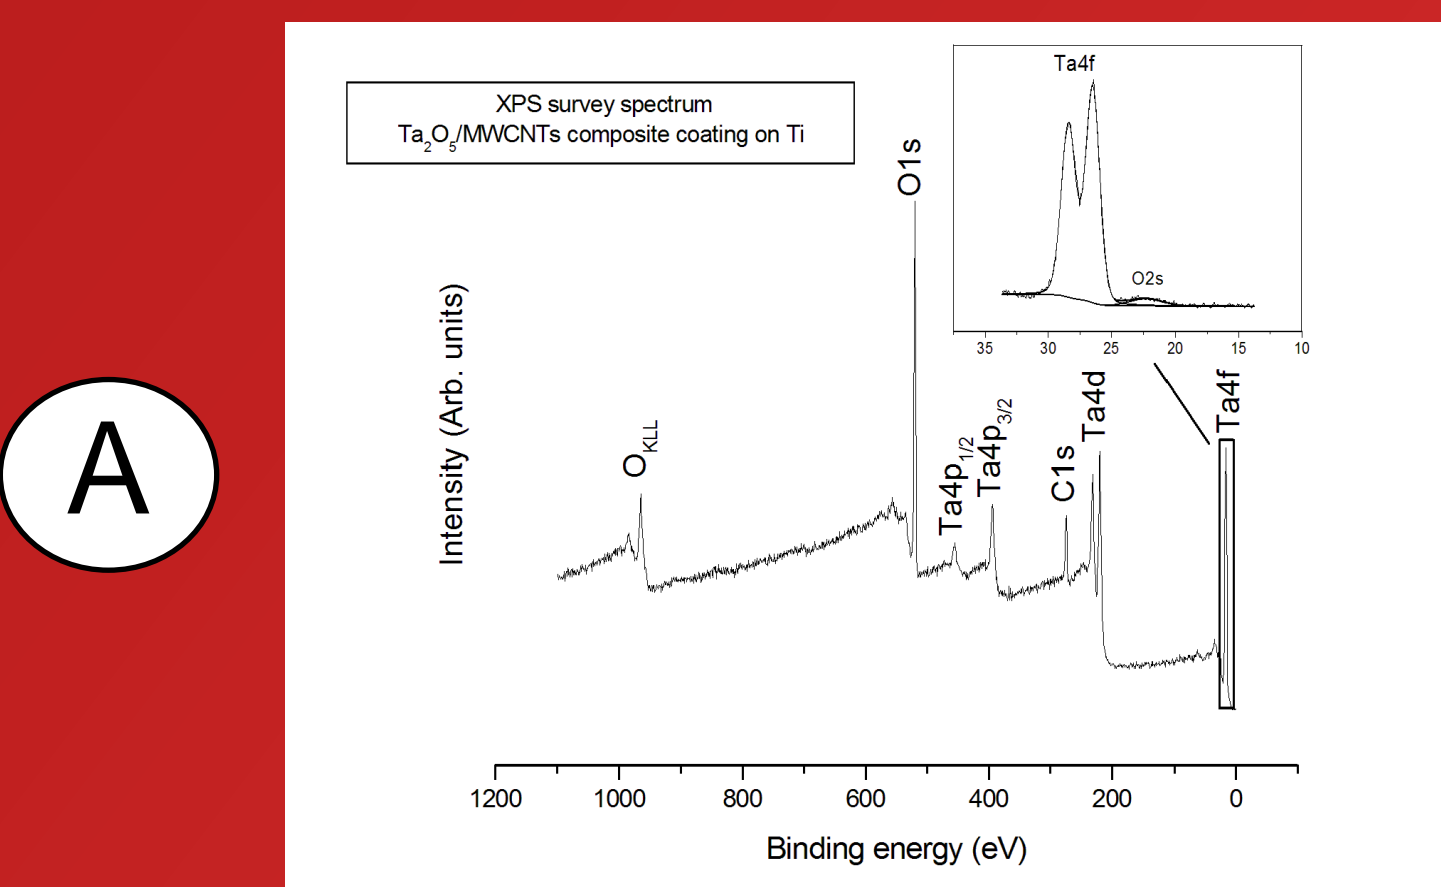

- => The optimized procedure allows the preparation of **high quality  $Ta_2O_5$ /MWCNTs composite coatings with great morphological, structural and adherent characteristics.**

### Functionalization with a molecular film of amino-tris-methylene phosphonic acid (B) and *in vitro* hydroxyapatite growth on a “completely-functionalized substrate: Ti/ $Ta_2O_5$ +MWCNTs/ $N(CH_2PO_3H_2)_3$ (C)

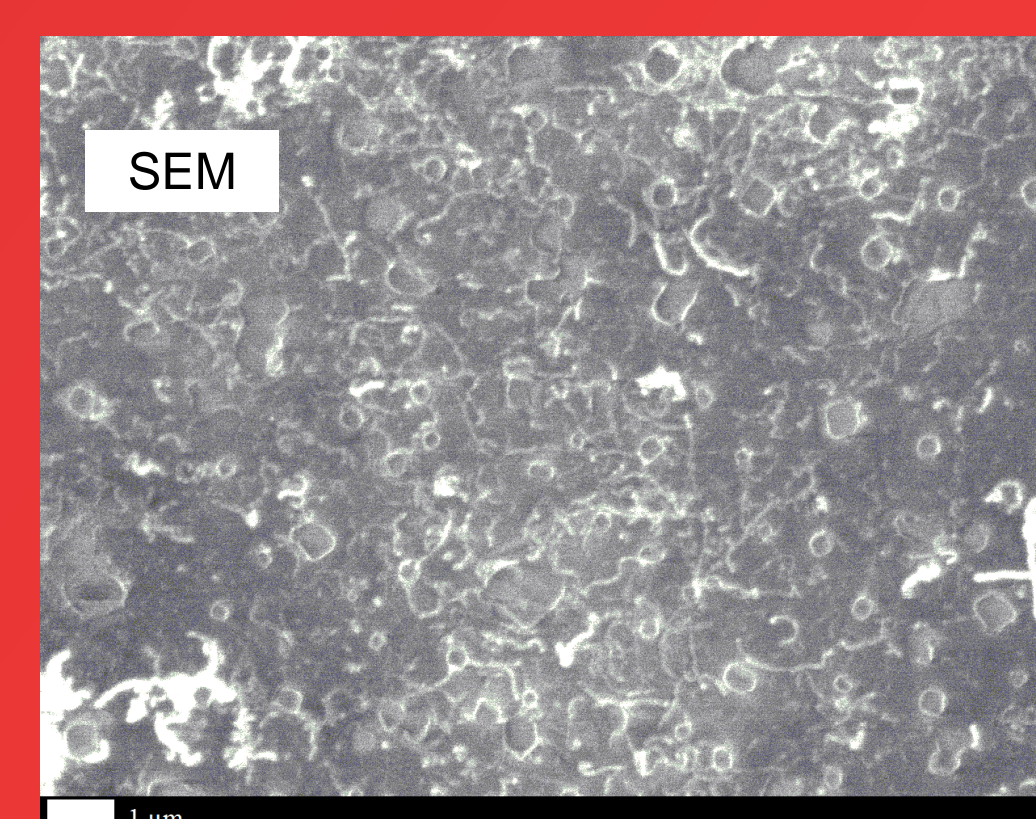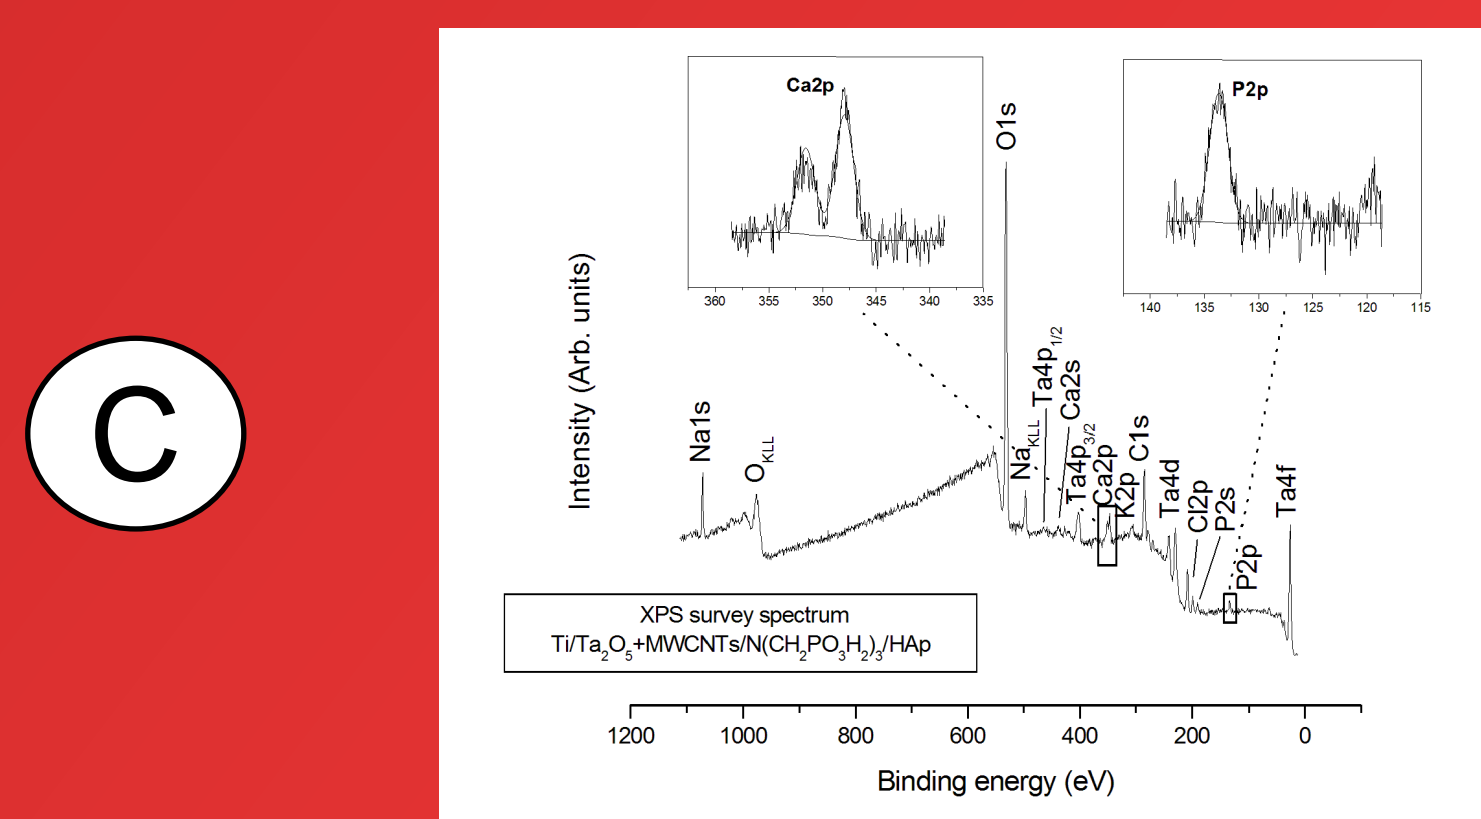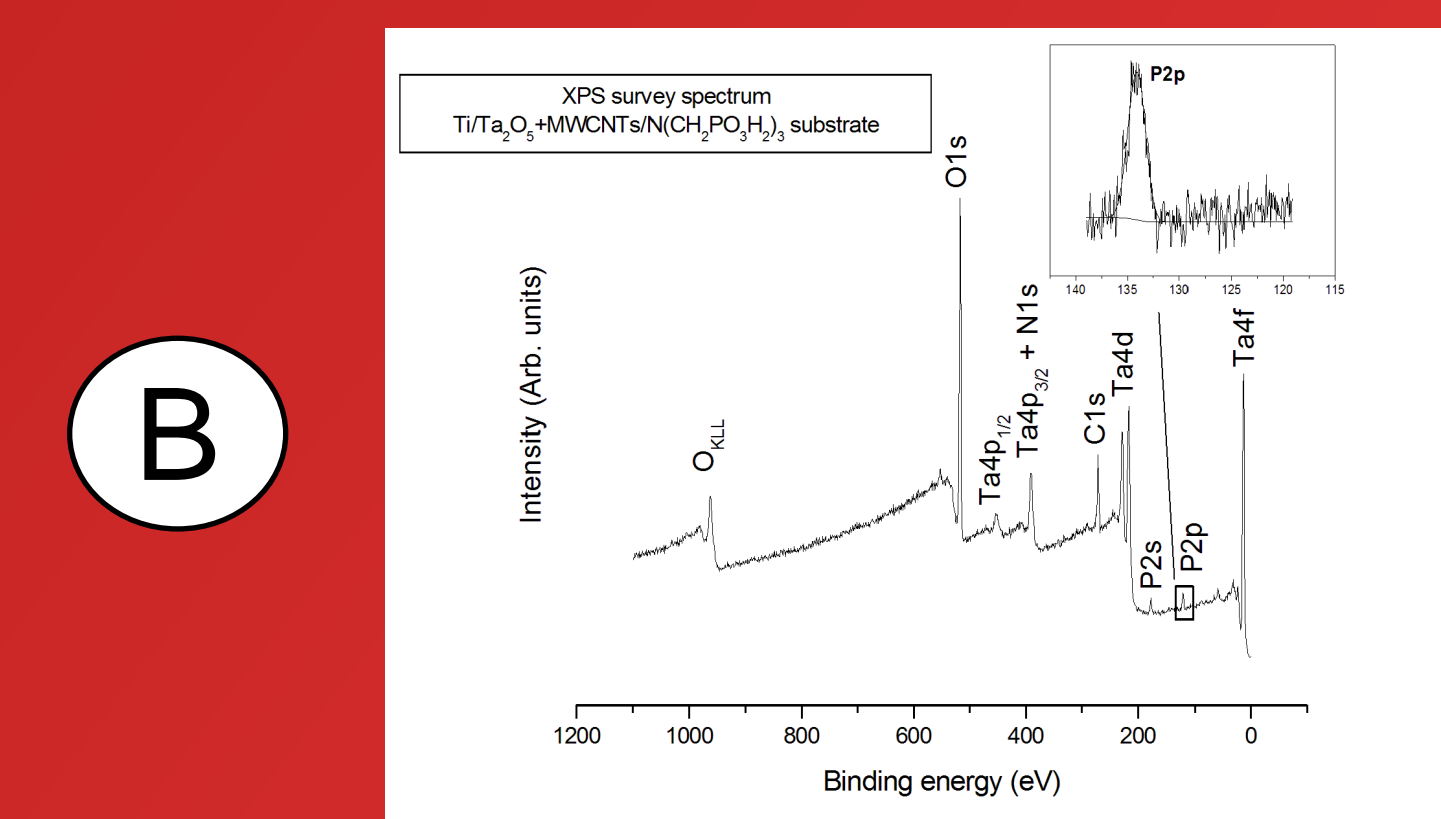

- => The presence of phosphonic acid molecules and hydroxyapatite is confirmed by XPS survey spectra.
- => SEM characterizations of « completely-functionalized » substrates reveal an **important density** of hydroxyapatite crystals with a **particularly well defined crystallinity** ( $\varnothing \sim 0.5 \mu m$ ).

## Conclusions and perspectives

- The considered approach allows the formation of **highly homogeneous, adherent and cracks-free tantalum-based deposits** on titanium which are particularly **resistant to corrosion**.
- The composite coating made of oxidized MWCNTs dispersed in a  $Ta_2O_5$  matrix, combined with the presence of surfacial phosphonic acid functions, leads to an **important reinforcement of the Ti substrate's bioactivity** through the *in vitro* formation of high quality hydroxyapatite crystals.
- Perspectives:** *in vitro* tests of proliferation and adhesion of osteoblasts, preparation of  $Ta_2O_5$ /MWCNTs composites on titanium and its alloys through electro(co)deposition, ...

## References

- M. Geetha, A.K. Singh, R. Asokamani, A.K. Gogia, *Prog. Mater. Sci.* **2009**, *54*, 397-425; N. Tran, T.J. Webster, *Wiley Interdiscip. Rev. Nanomed. Nanobiotechnol.* **2009**, *1*, 336-351.
- C. Arnould, T.I. Koranyi, J. Delhalle, Z. Mekhalif, *J. Colloid Interf. Sci.* **2010**, *344*, 390-394; V.K. Balla, S. Banerjee, S. Bose, A. Bandyopadhyay, *Acta Biomater.* **2010**, *6*, 2329-2334.
- P.J.F. Harris, *Inter. Mater. Rev.* **2004**, *49*, 31-43; N. Narita, Y. Kobayashi, H. Nakamura, K. Maeda, A. Ishihara, T. Mizoguchi, Y. Usui, K. Aoki, M. Simizu, H. Kato, H. Ozawa, N. Udagawa, M. Endo, N. Takahashi, N. Saito, *Nano Lett.* **2009**, *9*, 1406-1413.
- C. Arnould, C. Volcke, C. Lamarque, P.A. Thiry, J. Delhalle, Z. Mekhalif, *J. Colloid Interf. Sci.* **2009**, *336*, 497-503.