

RESEARCH OUTPUTS / RÉSULTATS DE RECHERCHE

Inter-laboratory variability of the standardized ETP-based APC resistance assay

Morimont, Laure; Didembourg, Marie; Haguët, Helene; Modaffari, Elise; Tillier, Maxence ;
Lebreton, Aurélien; Bouvy, Céline; Dogné, Jean-Michel; Douxfils, Jonathan

Published in:

ECTH 2021- Abstract Book, 14-15 October 2021

Publication date:

2021

[Link to publication](#)

Citation for pulished version (HARVARD):

Morimont, L, Didembourg, M, Haguët, H, Modaffari, E, Tillier, M, Lebreton, A, Bouvy, C, Dogné, J-M & Douxfils, J 2021, Inter-laboratory variability of the standardized ETP-based APC resistance assay. in *ECTH 2021- Abstract Book, 14-15 October 2021.*, P053, pp. 84, ECTH 2021, Gand, Belgium, 14/10/21.

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal ?

Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Inter-laboratory variability of the standardized ETP-based APC resistance assay

L. Morimont^{1,2}, M. Didembourg², H. Haguet², E. Modaffari¹, M. Tillier³, C. Bouvy¹, A. Lebreton³, J-M. Dogné², J. Doux fils^{1,2}

¹Qualiblood sa, Namur, Belgium; ²University of Namur, Faculty of Medicine, Department of Pharmacy, Namur Research Institute for Life Sciences (NARILIS), Namur Thrombosis and Hemostasis Center (NTHC), Namur, Belgium; ³Service d'hématologie biologique, CHU Clermont-Ferrand, Clermont-Ferrand, France.

Laure.morimont@qualiblood.eu

BACKGROUND

- Regulatory bodies recommend assessing the impact of steroid contraceptives on ETP-based APC resistance assay during their development.
- This assay was recently validated and standardized.


AIMS

To assess the inter-laboratory transferability of the ETP-based APC resistance assay.

METHODS

The study scheme is described in **figure 1**

Figure 1: Study scheme for the transferability of the ETP-based APC resistance assay

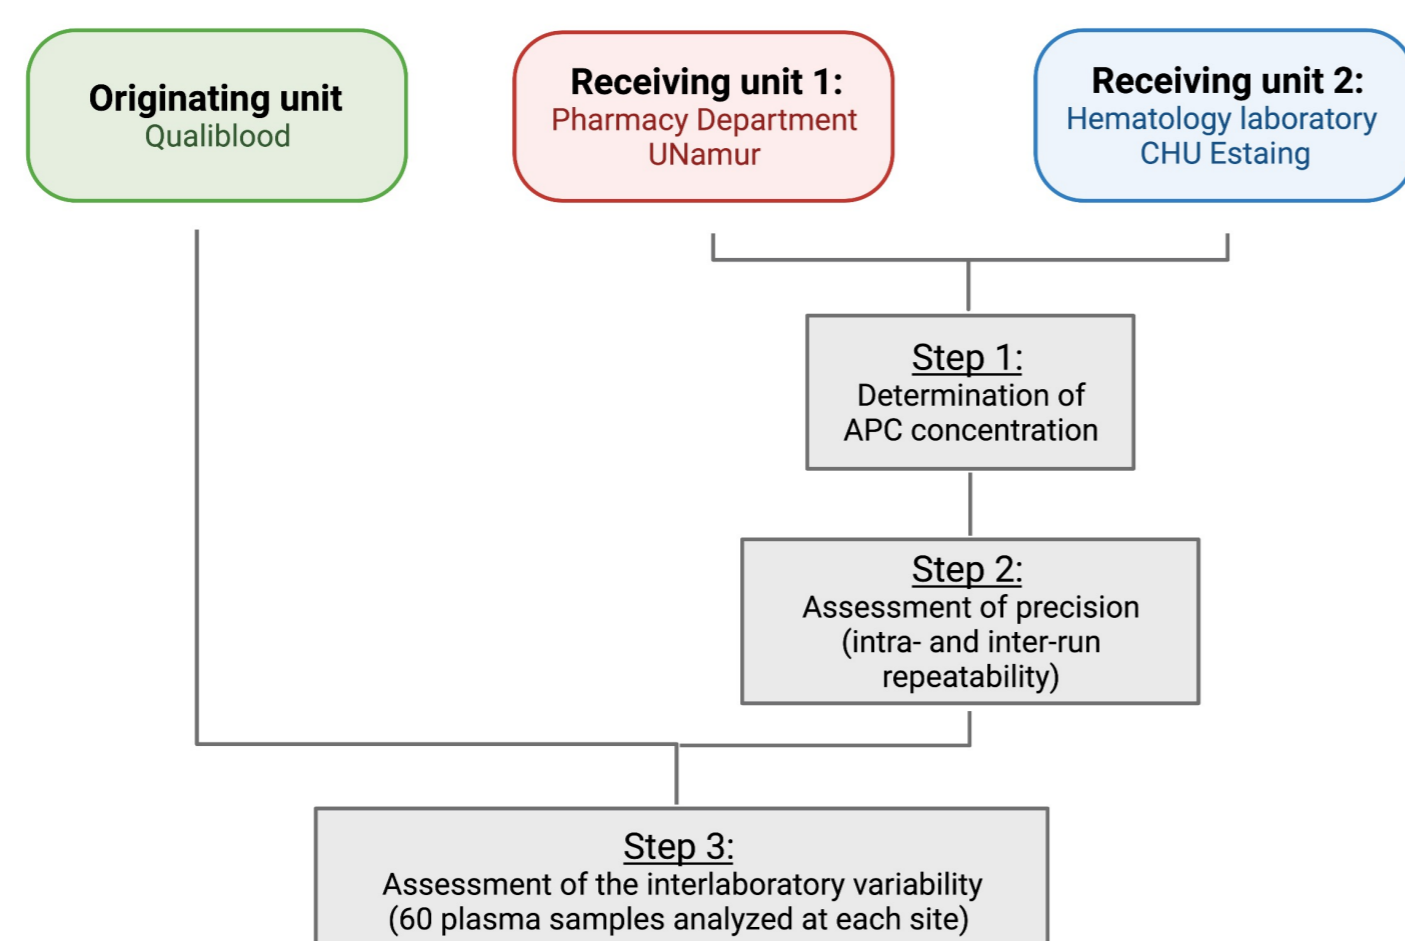

RESULTS

- APC concentration was defined at 1.21 µg/mL and 1.14 µg/mL in receiving unit 1 and receiving unit 2 respectively.
- Intra- and inter-run (**Table 1**) repeatability showed SD below 3% in both receiving units.
- Spearman correlation showed effective pairing between the originating and the receiving units (**Figure 2**).
- The sensitivity of the test was maintained and subgroups analysis still reported significant differences between healthy individuals and women using combined oral contraceptives (**Figure 3**).

SUMMARY/CONCLUSION

- Excellent intra-laboratory precision and inter-laboratory reproducibility.
- The normalized APC sensitivity ratio obtained with this validated methodology, provides an appropriate sensitivity irrespective of the laboratory in which the analysis is performed.

Table 1: Intra-run (N=5) and inter-run (N=3) repeatability (N=5) of the commercial reference plasma and the 3 quality controls. Results are expressed as mean inhibition % ± SD

Tested plasma	Intra-run repeatability		Inter-run repeatability	
	Unit 1	Unit 2	Unit 1	Unit 2
Reference plasma	78.8% ± 0.4%	75.3% ± 1.2%	80.9% ± 0.1.9%	78.5% ± 1.2%
QC low	100.0% ± 0.0%	100.0% ± 0.0%	100.0% ± 0.0%	97.9% ± 1.9%
QC intermediate	40.2% ± 0.7%	37.7% ± 0.9%	42.8% ± 2.6%	39.6% ± 2.3%
QC high	2.8% ± 0.7%	4.0% ± 1.5%	5.0% ± 2.3%	6.0% ± 2.1%

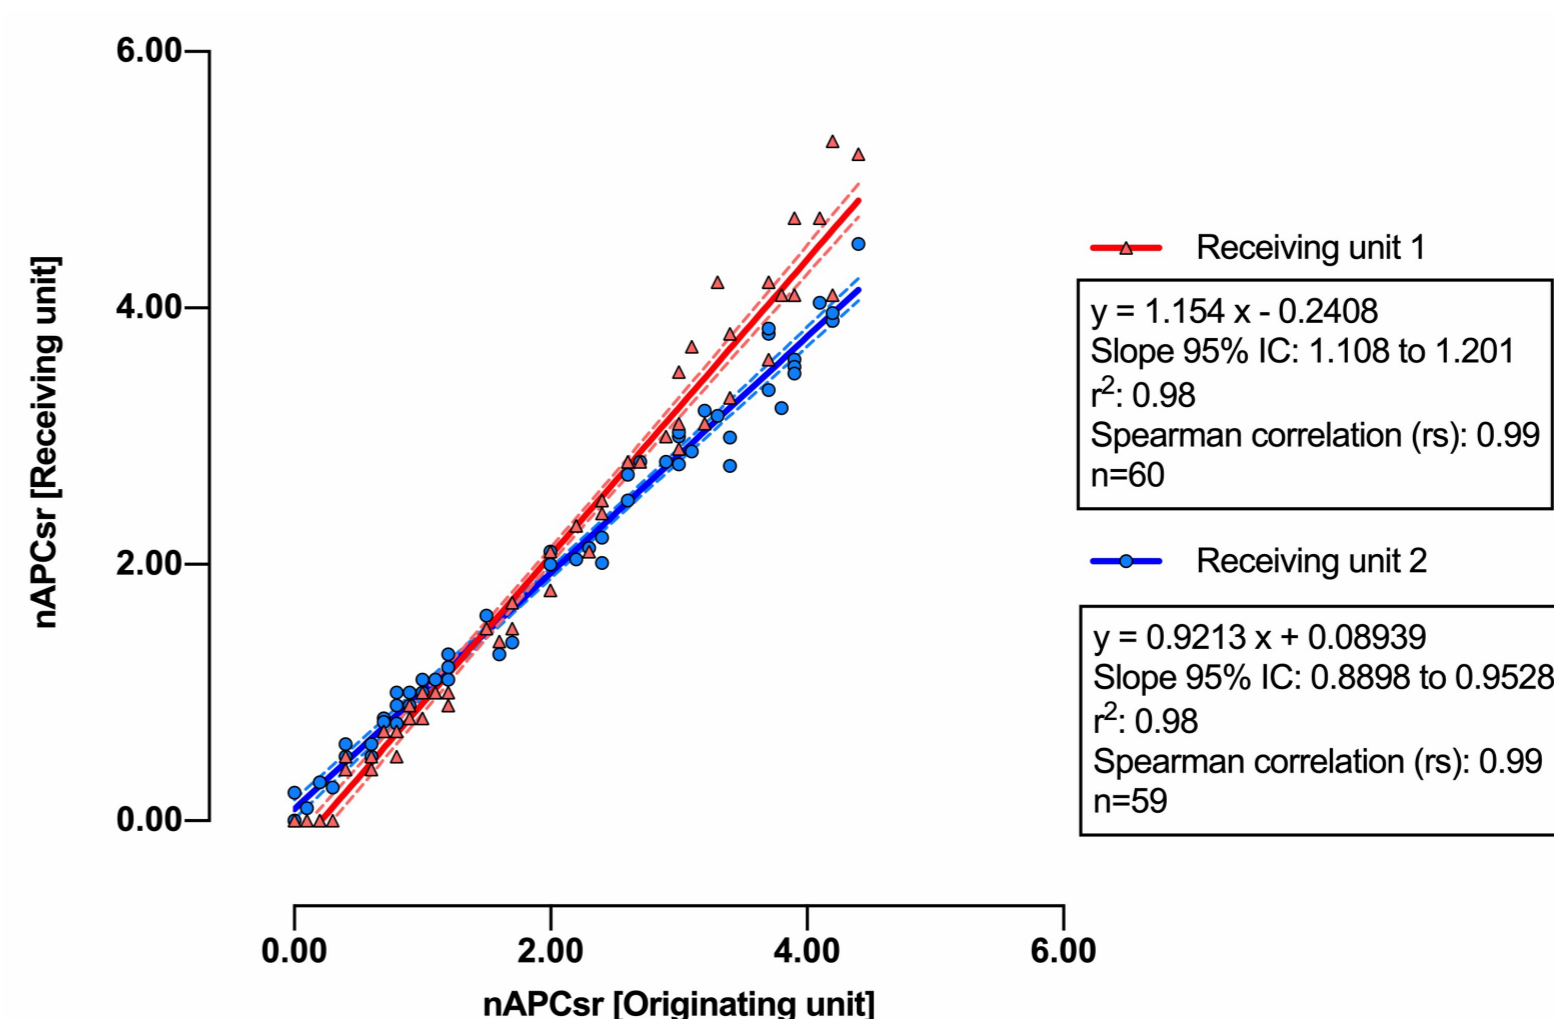


Figure 2: Correlation between normalized APC sensitivity ratio (nAPCsr) obtained at the receiving units and nAPCsr obtained at the originating unit.

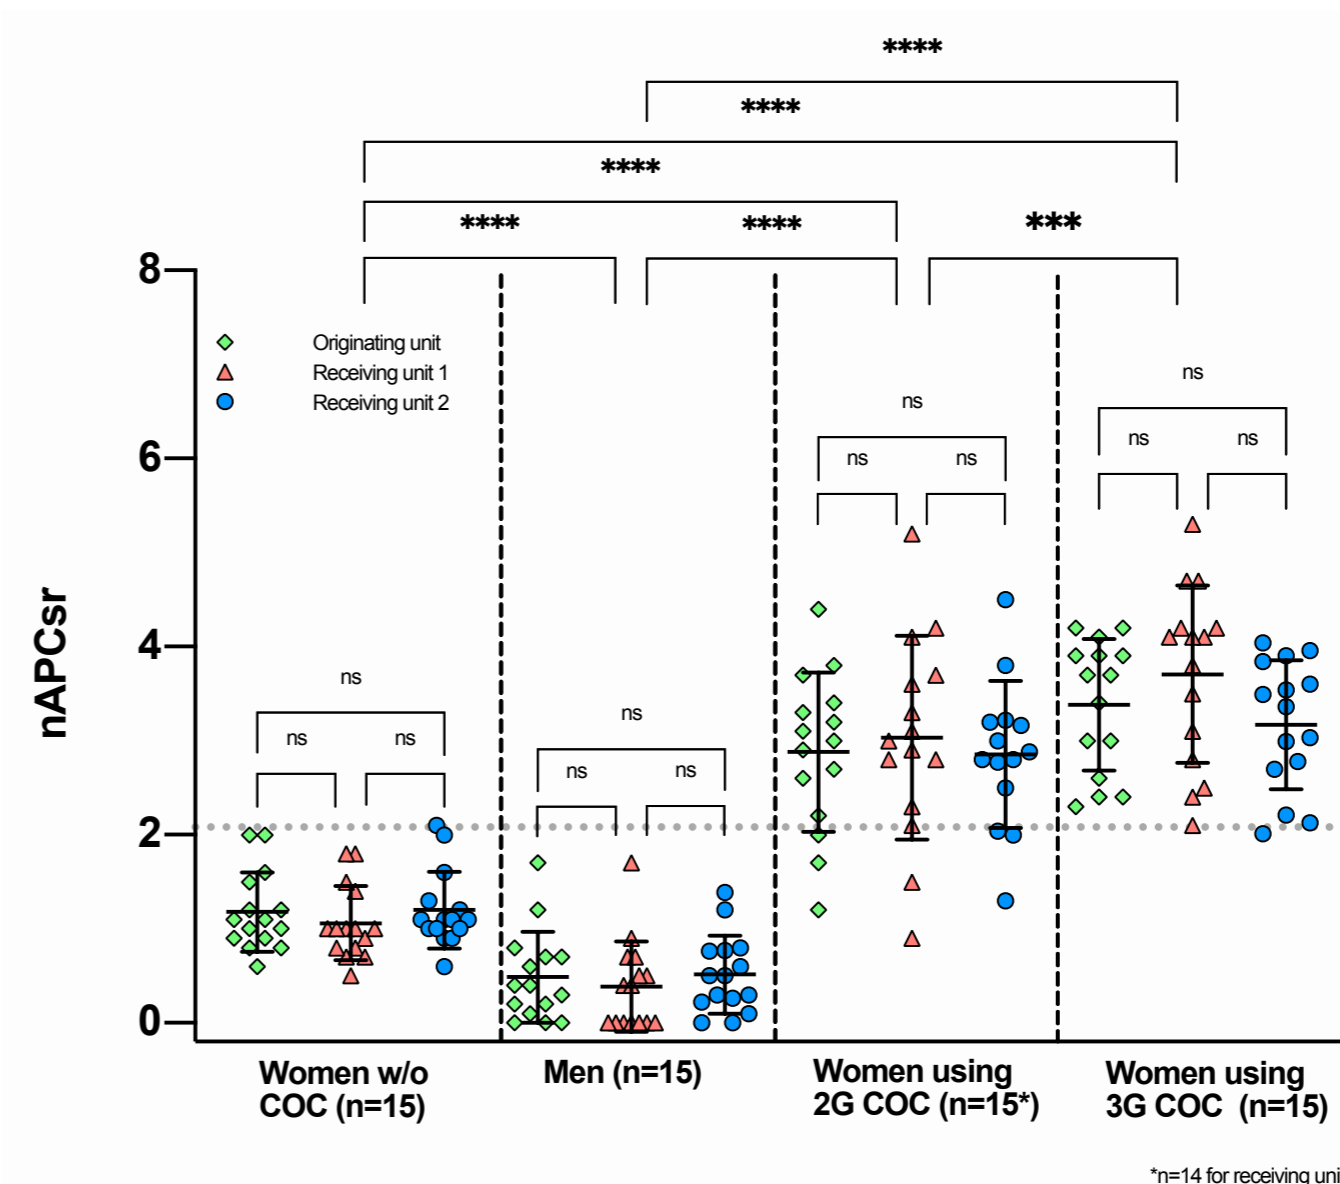


Figure 3: Normalized APC sensitivity ratio (nAPCsr) values of individuals from each subgroup (i.e., women without combined oral contraceptive (COC), men, women using 2nd generation (2G) COC and women using 3rd generation (3G) COC obtained at the different units.